



INSTRUCTION MANUAL

MT195

CABLE LOCATOR



Contents

Page no

Open-case Inspection	5
Safety Instructions	6
1. Overview	10
1.1 Product introduction	10
1.2 Characteristics of Cable Locator	11
1.3 Names and functions of parts	12
1.3.1 Sketch of transmitter	12
1.3.2 Transmitter display	12
1.3.3 Sketch of receiver	13
1.3.4 Receiver display	14
1.3.5 Display of receiver under cable locating mode	14
2. Carrying out measurement	15
2.1 Measurement precautions	15
2.2 Functional principle	15
2.3 Examples of typical application	17
3. Details of application	18
3.1 One-pole application	18
3.1.1 In open circuit	18
3.1.2 Locating and tracing of lines and sockets	19
3.1.3 Locating of line interruptions	20
3.1.4 Locating of line interruptions using two transmitters	21
3.1.5 Error detection for an electrical floor heating	22
3.1.6 Detect the narrow (blocked) part of the laid non-metallic pipeline	24
3.1.7 Detect the laid metal tap water pipe and metal heating pipe	25
3.1.8 Detect the power supply circuit on the same floor	26
3.1.9 Track an underground circuit	27
3.2 Dual-pole applications	28
3.2.1 Applications in closed circuits	28
3.2.2 Search for the fuses.....	29
3.2.3 Search for short circuit in the circuit.....	30
3.2.4 Detect circuits laid relatively deep	30
3.2.5 Classify or determine the laid circuit.....	32
3.3 Method to increase the effective radius of detecting charged circuits.....	33
3.4 Identify voltage in the grid and search for breakages in the circuit.....	34


Contents

Page no

4. Other functions.....	35
4.1 Voltmeter function of the transmitter.....	35
4.2 Flashlight function.....	35
4.3 Backlight function.....	35
4.4 Buzzer function.....	35
4.5 Automatic shutdown function.....	35
5. Technical parameters.....	36
5.1 Technical parameters of transmitter	36
5.2 Technical parameters of receiver	36
6. Repair and maintenance	37
6.1 Troubleshooting	37
6.2 Checking of the fuse of the transmitter	37
6.3 Cleaning	38
6.4 Replace the battery	38
6.5 Interval of calibration	39

Open-Case Inspection

When receiving this Cable Locator, please inspect it carefully to ensure no damage has occurred during transport. Generally accessories, control switches and connectors need to be checked. If there is any obvious damage or functional failure, please contact your supplier.

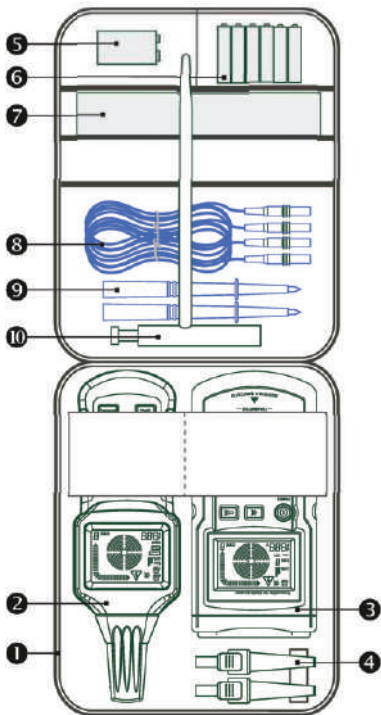

Main parts:

- 1 - CD Bag
- 2 - Receiver: 1 pcs
- 3 - Transmitter: 1 pcs

Accessories:

- 4 - Crocodile clamps:
2 pcs (respectively
red and black)
- 5 - Battery: 1 pcs
(9V alkaline battery,
GL6F22A 1604A)
- 6 - Battery: 6 pcs
(1.5V AAA alkaline
battery, LR03 SIZE)
- 7 - User's manual:
1 pcs
- 8 - Test leads: 2 pcs
(1.5m long,
respectively red
and black)
- 9 - Test probe: 2 pcs
(respectively red
and black)
- 10 - Grounding rod

Safety Information



WARNING

This Cable Locator is produced in accordance with the safety specifications for electronic meters and testing instruments and has been completely tested before packing and transport. Before using this device, please read this Manual carefully and follow all of the instructions. Failure to adhere to these instructions or ignoring the warnings and cautions herein may lead to injury, threat to life or damage of equipment.

Definition Of Safety Symbols

This Manual includes the basic elements for safe operation and maintenance of the cable locator. Before using the product, please read the following safety instructions carefully.

Table 1 : Safety Instructions

	Important information that users must read before using the product.
	Indicating that this terminal may be live.
	Conformity symbol.

Table 2 : Warning Instructions

 WARNING	Incorrect operation may cause serious hurt or death.
 CAUTIONS	Incorrect operation or carelessness may lead to personal hurt, damage of this cable locator or error in the measured results
 HINTS	Suggestions or tips for operation.



Attention!

Please observe the following instructions to ensure safe operation and optimal performance.

1. Preliminary Inspection

Before the first use, please check whether the cable locator can function normally and ensure it is not damaged during storage and transport. If there is any damage, please contact the supplier.




Whenever you use the Cable Locator, the related safety specifications in electronics industry must be abided by.

2. Placement

Temperature range for operation	0-40°C (32-104°C), <80%RH (non-condensation)
Temperature range for storage	-20-+60°C(-6-140°C F), <80%RH (non-condensation)

To avoid failures or incidents, please don't place the cable locator under the following environments:

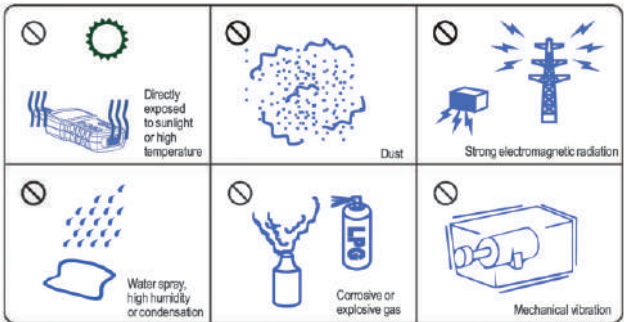

3. Use



The following instructions should be followed to avoid electric shock, short circuit or explosion:

1. This cable locator can be directly used for live parts, but do take insulation measures in accordance with industrial safety codes to avoid electric shock and hurt.
2. To avoid electrical shock, the valid safety and VOE regulations regarding excessive contact voltages must receive utmost attention, when working with voltages exceeding 120V (60V) DC or 50V (25V) rms AC. The values in brackets are valid for limited ranges (such as medicine and agriculture).
3. Never try to make contact between both battery cell poles, for example, by using a wire connection. Never throw the batteries into fire, otherwise there may be an explosion.
4. When replacing or changing the battery, make certain of correct polarity. Batteries with reversed polarity can lead to instrument destruction. Furthermore, they may explode or ignite.



1. Measurements in dangerous proximity of electrical installations only under the direction of a responsible electrician.
2. When the product is used for testing a live line, do ensure the test lead has been disconnected from the tested object before connecting or disconnecting the test lead of the transmitter.
3. Never try to disassemble battery cells! The battery contains very strong base chemicals. If the battery contents come in contact with skin or clothing, rinse immediately with water. If the battery contents come in contact with the eyes, immediately flush by using pure water and consult a doctor.
4. As the connection of the transmitter with the mains may generate a circuit current of milliampere levels, in live condition the Earth terminal of the transmitter can be only connected with a neutral conductor. If transmitter connection is from the phase towards the protective conductor, the functional safety of the protective conductor must be tested first, in compliance with DIN VDE 0100. The reason is that when connecting the transmitter from phase towards earth, all parts being connected to the earth may be live in the event of an error (if the earth resistance does not comply with the regulations).
5. If the operator's safety is no longer ensured, the instrument is to be put out of service and protected against use. The safety is no longer ensured, if the instrument:
 - ◆ shows obvious damage.
 - ◆ does not carry out the desired measurements.
 - ◆ has been stored for too long under unfavorable conditions.
 - ◆ has been subject to mechanical stress during transport.



6. The instrument may only be used under those conditions and for those purposes for which it was conceived. When modifying or changing the instrument, the operational safety is no longer ensured.



1. The working temperature of this Cable Locator is 0-40°C (32-104°F).
2. To avoid damage, this device should be protected against excessive mechanical vibration during handling or use, especially dropping.
3. Only qualified Technicians are allowed to calibrate and repair this instrument.
4. Prior to usage, inspect the instrument and the test lead in use for external damage. Please ensure that the instrument and the test lead in use are intact. The instrument should not be used unless all the functions of the instrument are well prepared for work.
5. When using the instrument, the rated voltage of the tested line should not exceed the rated voltage specified in the technical specifications of this Cable Locator.
6. Keep the instrument out of direct sunlight to ensure perfect functioning and long service life.
7. If the instrument is subject to an extremely high electromagnetic field, its functioning ability may be impaired.
8. Only use batteries as described in the technical data section.
9. Try to keep the battery away from humidity. If the display shows a flickering battery symbol, the batteries must be changed into new ones.



1. Before using a locator that has been placed or transported under extreme climate conditions, please place it under a new favorable environment for a certain period.
2. When the transmitter is connected with live mains, if the earth terminal of the transmitter is connected with protective earth phase, the current leakage (if any) in the power supply line may join the circuit current of the transmitter, leading to tripping of the leakage circuit breaker, i.e. tripping of FI/RCD.
3. Please maintain the original package well for later mailing (such as for calibration of the instrument).

1. OVERVIEW

1.1. Product Introduction

When you are making a hole in the wall for installation of an air conditioner or on the floor for installation of a machine, or excavating a road, you have to know the layout of the cables, water pipelines or gas pipelines in the wall or ground to keep away from these facilities and avoid unnecessary troubles and even dangers. In the past, there is only one solution for this issue, that is, to find the construction drawings of these embedded facilities. However, in most cases, these drawings cannot be found and you have to take your chance, which may result in interruption of cables or pipelines, bringing about the danger of power failure, electric shock, explosion or threat to life.

This Cable Locator will effectively assist users to locate and detect cables, accurately without having to guess the location.

This Cable Locator is a portable instrument consisting of a transmitter, a receiver and some accessories. With advanced integrated parts and digital circuit technologies, it is characterized by

highly stable and reliable electrical performance. The transmitter sends to the target cable (or metal pipes) an AC voltage modulated by digital signals, which generates an alternating electric field; Put the sensor head of the receiver close to this electric field, and the sensor will generate induced voltage. This instrument can magnify this weak voltage signal by hundreds of times and then display it via an LCD screen after audio frequency decoding, demodulation and digital processing, so that the position of the buried cables or pipes, as well as their faults, can be detected based on the change of the signal.

This Cable Locator is easy to use and provides convenient operation by means of push buttons, which indicate effective pressing through a buzzer. The display is visualized and the transmitter and receiver are equipped with LED lamps. The transmitter not only transmits signals but also acts as an AC/DC voltmeter, so that the instrument can display the voltage of the tested line, including the AC/DC status, in addition to a warning symbol when testing a live line.

The transmitter has a self check function which is shown in the display to show whether the transmitter is transmitting signals. The display of the receiver has backlights, so that users can see the testing results even in dark areas. To improve the testing efficiency, the receiver is equipped with a loudspeaker, which will give changing tones at the time of changed signal intensity, so that users can judge the testing effects simply by sound. In mute mode for both the transmitter and the receiver is provided to prevent them from disturbing others when the instrument is used.

This Cable Locator is applicable for construction involving telecommunication cables, power cables and building pipelines, as well as maintenance of such cables and pipelines.


1.2. Characteristics of This Cable Locator

- Detecting cables, electrical lines, water/gas supply pipelines in walls or underground;
- Detecting interruptions and short circuit in cables and electrical lines in walls or underground;
- Detecting fuses and assigning current circuits;
- Tracing sockets and distribution sockets that have accidentally been covered by plastering;
- Detecting interruptions and short-circuits under floor heating;
- The transmitter is integrated with the function of AC/DC voltmeter, which can measure 12 to 400V
AC/DC voltage on a linear basis:
AC ~ : 12 to 400V (50 to 60 Hz)± 2.5%
DC ---: 12 to 400V ± 2.5%
- The screen of the transmitter can display preset transmitting power, transmitted codes, its own battery energy, mains voltage detected, AC/DC status of mains voltage detected, and warning symbol for mains voltage.
- The transmitter has a self check function to detect its own working status and to display it on the LCD screen for user's reference.
- The screen of the receiver can display the transmitting power of the transmitter, transmitted codes, energy of the transmitter's and its own batteries, AC voltage induced signal detected and warning symbol for mains voltage.
- The sensitivity of the receiver can be adjusted either manually or automatically.
- The receiver can sweep frequency automatically.
- Both the transmitter and the receiver can work under mute mode.
- The receiver is available with auto power off (It is powered off automatically over 10 minutes of if there are no buttons pressed).
- The receiver's LCD screen is provided with backlight for application in poor light.
- Both the transmitter and the receiver is provided with flashlight function when working in dark areas.
- Additional transmitters are available to extend or distinguish several signals.
- Compact, durable and portable.

1.3. Names And Functions Of Parts


1.3.1. Sketch of transmitter

- 1 - LCD screen.
- 2 - Power on/off key.
- 3 - Key for setting/confirming transmitting power level (Level I, II or III)
- 4 - Key for transmitting or stopping to transmit code information.
- 5 - Key for setting/confirming code information to be transmitted. Press this key for 1 second to enter code setting and press it briefly to exit setting (Code F, E, H, D, L, C, 0 or A can be selected, with default as F).
- 6 - Down key. When setting power level or code, press it to go down.
- 7 - Up key. When setting power level or code, press it to go up.
- 8 - Key for enabling or disabling mute mode (no keypad tone under mute mode).
- 9 - Key for turning on/off flashlight.
- 10 - "+" hole, input/output hole of the transmitter. The transmitter is connected to external cables with the test lead through this hole to send out signals and receive detected voltage signals.
- 11 - Earth Terminal. The transmitter is grounded with the test lead through this hole.

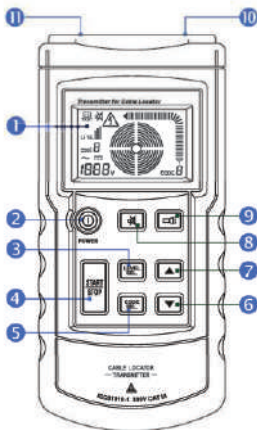


1.3.2. Transmitter display

- 1 - Symbol to indicate voltage/energy of the transmitters battery.
- 2 - Transmitting power level (Level I, II or 111)
- 3 - Transmitting code (default as F).
- 4 - Mains AC voltage
- 5 - Mains DC voltage
- 6 - Mains voltage value (can be used as an ordinary voltmeter; range: 12 to 400v DC/AC)
- 7 - Transmitting status.
- 8 - Code being transmitted.
- 9 - Intensity of signal being transmitted.
- 10 - Symbol to indicate mains voltage.
- 11 - Symbol to indicate mute mode.




1.3.3. Sketch of receiver

- 1 - Flashlight.
- 2 - Probe head
- 3 - LCD screen
- 4 - Power on-off key
- 5 - Composite key for backlight and mute mode. Press briefly to enable/disable backlight and press for 1 second to enable/disable mute mode (under mute mode, both the keypad tone and the speaker are silent).
- 6 - Key for turning on/off the flashlight.
- 7 - UAC key for switchover between cable locating mode and mains voltage.
- 8 - MANUAL key for switchover between manual and automatic cable locating.
- 9 - Key for adjusting sensitivity down under manual mode.
- 10 - Key for adjusting sensitivity up under manual mode.
- 11 - Loudspeaker.

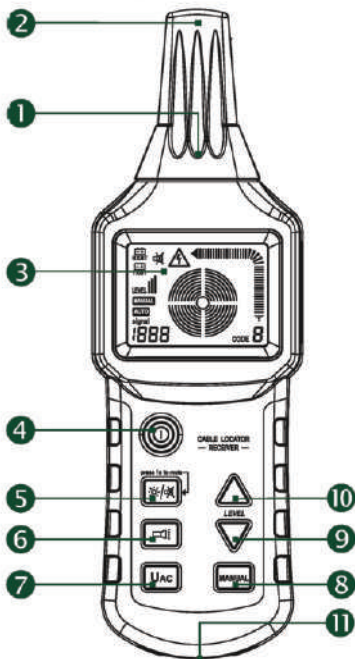

1.3.4. Receiver display

- 1 - Symbol to indicate voltage/energy of the receiver's battery.
- 2 - Symbol to indicate voltage/energy of the transmitter's battery.
- 3 - Transmitting power level received (Level I, II or 111)
- 4 - Symbol of manual mode.
- 5 - Symbol of automatic mode.
- 6 - Automatic mode, this number indicates signal intensity; under manual mode, this place displays SEL to indicate no signal or displays a number indicating the signal intensity; under UAC mode, this place displays "UAC".
- 7 - Concentric circles indicating the preset sensitivity in graphics. More circles indicate higher sensitivity, while fewer circles indicate lower sensitivity.
- 8 - Code received.
- 9 - Intensity of signals.
- 10 - Symbol to indicate mains voltage.
- 11 - Symbol to indicate mute mode.

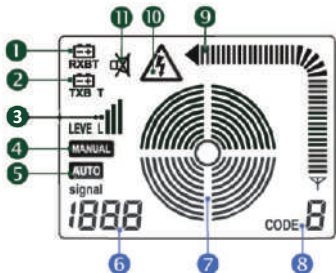

1.3.5. Display of receiver under cable locating mode


1. Automatic mode



2. Manual mode



3. Mains voltage identification mode



2. Measuring Method

2.1. Measurement Precautions



1. As the connection of the transmitter with the mains supply may generate circuit current of milliamperes, in a live condition the earthing of the transmitter can be only connected with a neutral conductor. If transmitter connection is connected from the phase towards the protective conductor, the functional safety of the protective conductor must be tested first, in compliance with DIN VDE 0100. The reason is that when connecting the transmitter from phase towards earth, all parts being connected to the earth may be live in the event of an error (if the earth resistance does not comply with the regulations).
2. When the transmitter is connected with live mains, if the earth of the transmitter is connected with protective earth, the current leakage (if any) in the power supply line may increase the circuit current of the transmitter, leading to tripping of the leakage circuit breaker, i.e. tripping of FI/RCD.



1. When the transmitter as a voltage tester to test the mains voltage, it may arc when the probes touch the mains voltage, this is normal phenomenon.
2. If any one of the "Start/Stop" button, the "Code Set" button and the "Level Set" button is effective, the other two are ineffective.
3. If the receiver is under automatic mode, it can be switched to manual mode or mains voltage identification mode at any time; if the receiver is under manual mode, either UAC button or MANUAL button will be effective only upon quitting from the manual mode.

2.2. Functional principle

This Cable Locator consists of a transmitter, a receiver and accessories. The transmitter sends an AC voltage modulated by digital signals, which generates an alternating electric field to the target cable (or metal pipes) (see Fig. 2-1); Put the probe of the receiver close to this electric field, and the sensor will generate induced voltage. This instrument can magnify this weak voltage signal by hundreds of times and then display it via a LCD screen after digital processing, so that the position of the buried cables or pipes, as well as their faults, can be detected based on the change of the signal.



For any application, the connections of the transmitter should ensure a closed circuit. £11 2. This Cable Locator can only detect or locate lines correctly connected in accordance CAUTIONS to the physical principle described.

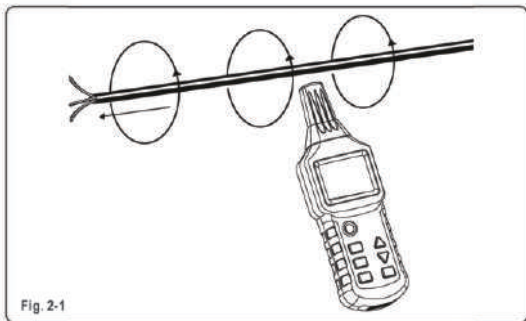


Fig. 2-1

Alternate connections of this Cable Locator

1. One-pole application: Connect the transmitter to only one conductor. Due to the high-frequency signal generated by the transmitter, only one single conductor can be located and traced. The second conductor is the earth. This arrangement causes a high frequency current to flow through the conductor and to be transmitted to the earth, similar to a radio or a receiver.
2. Double-pole application: The transmitter is connected to the conductor by two test leads. This application includes live mains and disconnected mains.

- The transmitter connected to live mains: Connect the "+" terminal of the transmitter to the phase line of mains and the Earth terminal of the transmitter to the neutral line of the mains. Under this circumstance, if there is no load in the mains, the modulated current from the transmitter will go to the neutral line via coupling through the distributed capacitance in the mains and then return to the transmitter.
- The transmitter connected to disconnected mains: Connect the "+" terminal of the transmitter to a terminal of a line in the mains, connect the Earth terminal to the terminal of another parallel line in the mains, and then





connect the other two terminals in the mains with each other. Under such circumstance, the modulated current will directly return to the transmitter through the mains. Optionally, the two test leads of the transmitter can be respectively connected to the two ends of the conductor. Besides, the "+" terminal of the transmitter can be connected to a terminal in the mains while the Grounding hole of the transmitter can be connected to the protective earth terminal of the mains.

2.3 Examples of Typical Application

In this example, please take a piece of a shielded cable with a cross sectional area of 1.5mm². Provisionally install 5m of this cable along the wall with nail clips at eye level as surface mounting. Make sure that the wall is accessible from both sides. Create an artificial interruption at a distance of 1.5m before the line terminal. The line terminals must be open. Strip the interrupted lead at the beginning of the light shielded cable and connect it via the test leads (provided) with terminal ⑩ of the transmitter. Connect terminal ⑪ of the transmitter to a suitable earth. All other cable leads must also be connected to the transmitter and the same earth (See Fig. 2-2). Switch on the transmitter via button ②, when the LCD screen of the transmitter displays the initial screen the buzzer will buzz. Press button ③ of the transmitter to enter the screen for setting transmitting level and then press up button ⑦ or down button ⑥ to select transmitting power level (Level I, II or III). After this level is set, press button ③ to exit. If you want to change the transmitting code, press button ⑤ of the transmitter for about 1 second and then press up button ⑦ or down button ⑥ to select transmitting code (F, E, H, D, L, C, 0 or A, with default F). Press button ⑤ to exit. Then, press button ④ to send information. At this moment, the concentric circles ⑦ on the LCD display will be gradually spread, and symbol ⑧ will display the transmitting code received by the transmitter itself, and symbol ⑨ will display the signal intensity. Press key ④ of the receiver to power on the receiver, when the LCD screen of the receiver displays the initial screen, the buzzer will buzz, and the receiver will enter the default "Automatic Mode". Move the probe of the receiver slowly along the cable to the interruption position, the symbol ③ of the receiver will display transmitting power level, ⑧ will display the code transmitted by the transmitter, ⑨ will display the dynamic signal intensity, and the speaker will change tone with the change in signal intensity.

When the probe of the receiver passes the interruption position, the signal intensity as displayed by ⑨ and ⑥ will have an obvious drop till it completely disappears. At this moment, press MANUAL button ⑧ of the receiver to switch it to manual mode and then use button ⑨ and ⑩ to reduce the sensitivity as much as possible while ensuring that ⑧ the receiver's screen can display the code transmitted by the transmitter. Then, this area is where the interruption is located.

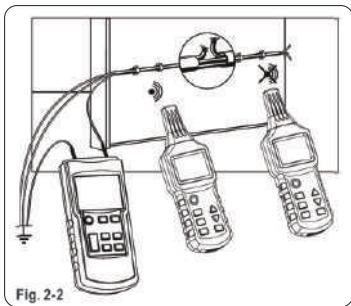


Fig. 2-2

1. Proper or good earth should be ensured.
2. Adjust the transmitting power level of the transmitter to adapt it to different detection radiuses. The best practice for testing is to mark the interruption position on the other side of the wall. Press MANUAL key of the receiver to switch it to manual mode. Press button ⑨ and ⑩ to reduce the sensitivity to make sure that the signal is just receivable. Trace the signal in front of the wall with the receiver till it is no longer indicated

3. DETAILS OF APPLICATION

3.1. One-Pole Application

3.1.1. In Open Circuit

- Detecting line interruptions in wall or floor;
- Finding and tracing lines, sockets, junction boxes, switches, etc. for house installations;
- Finding bottlenecks, kinking and buckling and obstructions in installation pipes by means of a metal wire.



When using this application, please ensure the you have a proper or good earth.



1. Application in open circuit is suitable for finding sockets and switches in disconnected equipment.
2. The tracing depth is depending on the medium and application. A typical tracing depth is D to 2m. The protective terminal of an electrical outlet can be used as the earth connection of the transmitter.

3.1.2. Locating and tracing of lines and sockets

Preconditions:

- The circuit must be dead or disconnected.
- Neutral line and protective earth wire must be connected and fully operational.
- Connect transmitter to phase line and protective earth wire according to Fig. 3-1-2.

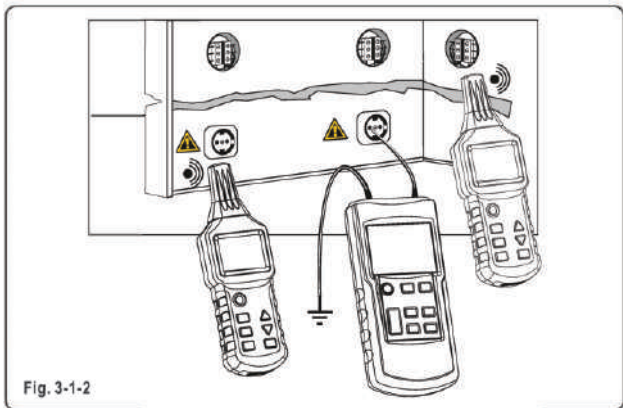


Fig. 3-1-2



HINTS

1. Proper or good earth should be ensured.
2. With the one-pole indication, also parallel circuit branches can be traced (The breaker must be removed in this example).
3. If the supply cable fed with the signals via the transmitter is located, e.g. directly in parallel to other conductors (e.g. cable groove or duct), or these conductors are crossed, the signals are also input into the other conductors.
4. During locating and tracing, the stronger the signal displayed, the closer the locator is to the lines to be traced.
5. Adjust the transmitting power level of the transmitter to adapt it to different detection radii.
6. The target position can be precisely located by your setting of the manual mode of the receiver and selecting of proper sensitivity.

3.1.3. Locating of line interruptions

Preconditions:

- The circuit must be dead or disconnected.
- All lines which are not required must be connected to the auxiliary earth in accordance with Fig. 3-1-3.
- Connect the transmitter to one lead and to an auxiliary earth according to Fig. 3-1-3.

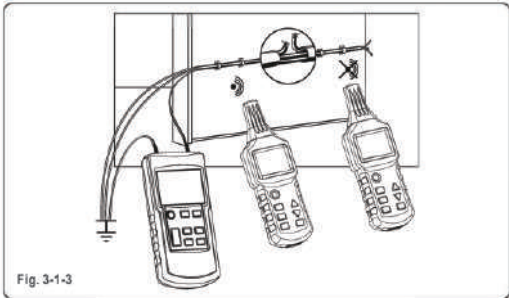


Fig. 3-1-3



1. Proper or good earth should be ensured.
2. The transition resistance of a line interruption must be higher than 100kOhm.
3. When tracing line interruptions in multi-core cables, note that all remaining leads in the shielded cable or conductor must be earthed in accordance with the regulations. This is required to avoid cross-coupling of the fed signals (by a capacitive effect to the source terminals). The tracing depth for shielded cables and conductors are different, as the individual leads in the shielded cables are twisted around themselves.



1. The earth connected to the transmitter can be an auxiliary earth, earth from an earthed socket or a water pipe which is properly earthed.
2. During tracing along the line, the position at which the signal received by the receiver has an abrupt decline is the position of the interruption.
3. Adjust the transmitting power level of the transmitter to adapt it to different detection radiuses.
4. The target position can be precisely located by your setting of the manual mode of the receiver and selecting of the proper sensitivity.

3.1.4. Locating of line interruptions using two transmitters

When locating a line interruption using one transmitter to feed from one conductor end, the location of the interruptions may not be precisely located in case of bad conditions due to a field disturbance. The drawbacks described above can easily be avoided when one uses two transmitters (one from each end) for line interruption detection. In this instance, each of the transmitters are set to a different line code, e.g. transmitter one to code F and the other to code C. (A second transmitter with a different line code is not included within the scope of supply and, therefore, has to be ordered separately.)

Preconditions:

- The current circuit must not be live.
- All lines not being used must be connected to the auxiliary earth as shown in Fig. 3-1-4.
- Connect both transmitters as shown in Fig. 3-1-4.
- Proceed as described in the application example.

If the transmitters are connected in accordance with Fig. 3-1-4, the receiver indicates Con on the left side of the line interruption. If the receiver goes beyond the interruption position towards the right, it will display F. If you are directly above the interruption, no line code is displayed, due to the overlapping of both transmitter signals.

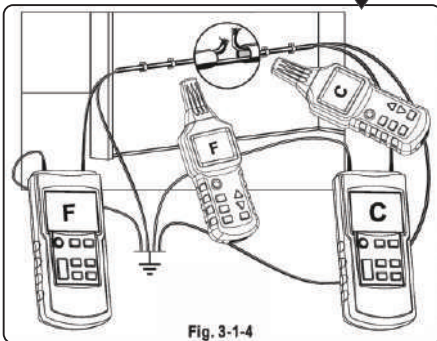


Fig. 3-1-4



1. Adjust the transmitting power level of the transmitter to adapt it to different detection radiuses.
2. The target position can be precisely located by your setting of the manual mode of the receiver and selecting of the proper sensitivity.




1. Proper or good earth should be ensured.
2. The transition resistance of a line interruption must be higher than 1 00kOhm.
3. The earth connected to the transmitter can be an auxiliary earth, earth from an earthed socket or a water pipe which is properly earthed.
4. When tracing line interruptions in multi-core cables, note that all remaining leads in the shielded cable or conductor must be earthed in accordance with the regulations. This is required to avoid cross-coupling of the fed signals (by a capacitive effect to the source terminals). The tracing depth for the shielded cables and conductors are different, as the individual leads in the shielded cables are twisted around themselves.

3.1.5. Error detection for an electrical floor heating

Preconditions:

- The current circuit must not be live.
- All lines not being used must be connected to the auxiliary earth as shown in Fig. 3-1-5a.
- Connect both transmitters (if two transmitters are used) as shown in Fig. 3-1-5b.
- Proceed as described in the application example.

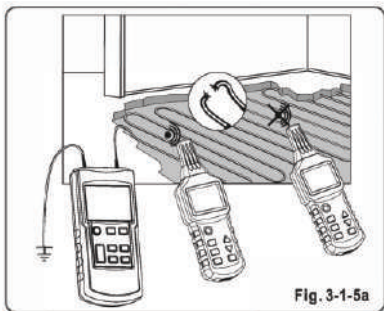

1. If a shield mat is located above the heating wires, no earth connection may exist. If required, separate the shield from the earth connection.
2. Proper or good earth should be ensured, and there should be considerable distance between the earthing terminal of the transmitter and the target line. If this distance is too short, the signal and line cannot be precisely located.

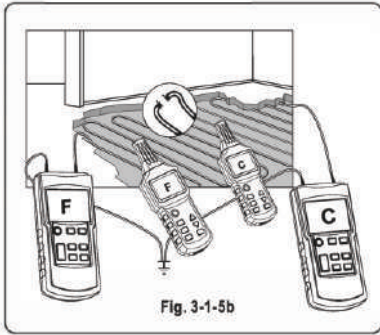


Fig. 3-1-5b

1. During tracing along the line, the position at which the signal received by the receiver has an abrupt decline is the position of the interruption.
2. Adjust the transmitting power level of the transmitter to adapt it to different detection radiuses.
3. The target position can be precisely located by your setting of the manual mode of the receiver and selecting of the proper sensitivity.
4. A second transmitter is not absolutely necessary for this application. For single transmitter application, see Fig. 3-5-1a.

3.1.6. Detect the narrow (blocked) part of the laid non-metallic conduct

Preconditions:

- The conduit must be made of non-conductive materials (such as plastic);
- The conduit must not be charged;
- The transmitter is connected to a metal helical tube (metal tube or flexible conduit) and an auxiliary earth wire, as shown in Fig.3-1-6;
- The measuring method is the same as that used in the example.

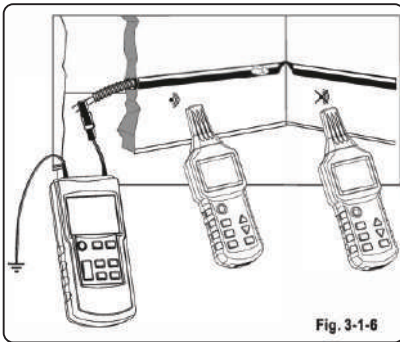


Fig. 3-1-6

1. If there is current in the conduit, disconnect the power, and correctly earth.
2. The earth should be properly connected and the transmitter earth should be a certain distance away from the conduct to be measured. If the said distance is too short, the signal and the circuit cannot be precisely located.



HINTS

1. If you only have one flexible tube that is made of non-conductive material (such as made of PVC) conduit, we suggest that you insert a metal wire with the section area of about 1.5mm² into the non-conductive conduct, and then push it into the narrow part.
2. In the process of detecting the conduit, the stronger the signals displayed on the receiver the closer the pipe is detected by the detector.
3. In the process of detecting along the conduit, if the signals received by the receiver is suddenly attenuated, the detected position is where the blockage locates.
4. Adjust the transmitting power of the transmitter to adapt to different radiuses of detection. Select the manual mode on the receiver and select suitable receiving sensitivity to precisely locate the narrow part.

3.1.7. Detect the laid metal water pipe and metal heating pipe

Preconditions:

- The pipe must be made of metal materials (such as galvanized steel pipe);
- The pipe to be detected should not be earthed. There should be a relatively high resistance between the pipe and the soil (otherwise the distance of detection will be very short);
- Use a connection wire to connect the earth probe on the transmitter to the earth, and property earth the end;
- Use a connection wire to connect the '+' socket on the transmitter to the pipeline to be detected.

The detection of laid water pipe is shown in Fig.3-1-7a and Fig.3-1-7b respectively:



CAUTIONS

For the sake of safety, the power supply of electrical equipments must be turned off.

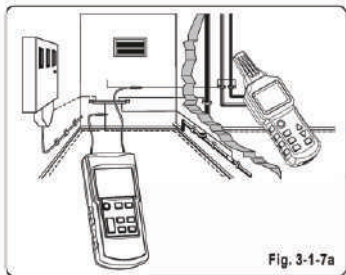


Fig. 3-1-7a

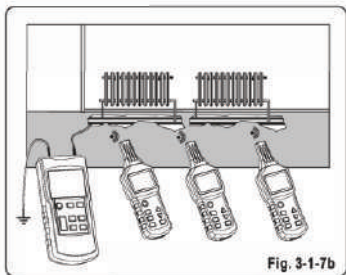


Fig. 3-1-7b




HINTS

1. The earth probe of the transmitter should be a certain distance away from the water pipe to be detected. If the distance is too short, the signals and the circuit cannot be precisely located.
2. Adjust the transmitting power of the transmitter to adapt to different radiuses of detection.
3. In the process of detecting the water pipe, the stronger the signals displayed on the receiver head of the detector, the closer the pipeline detected by the detector.
4. Select the manual mode on the receiver and select suitable receiving sensitivity to precisely locate the pipe.
5. To detect a pipe that is made of non conductive materials, it is suggested to insert a metal wire into the pipeline first, as described in Section 3.1.6.

3.1.8 Detect the power supply circuit on the same floor

When detecting the power supply circuit on the same floor, please take the following steps:

1. Turn off the main switch in the distribution box of this floor;
2. Disconnect the neutral wire in the distribution box of this floor from the neutral wires of other floors;
3. Connect the transmitter in a way shown in Fig.3-1-8.

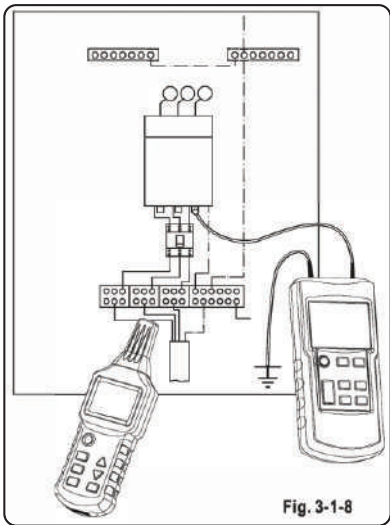

WARNING

For the sake of safety, please disconnect the power of the whole building.



HINTS

1. The earth probe of the transmitter should be properly earthed, and should be a certain distance away from the pipeline to be detected. If the distance is too short, the signals and the circuit cannot be precisely located.
2. Adjust the transmitting power of the transmitter to adapt to different radiuses of detection.
3. In the process of detecting and tracking the pipeline, the stronger the signals displayed on the receiver of the detector, the closer the supply is detected by the detector.
4. Select the manual mode on the receiver and select suitable receiving sensitivity to precisely locate the supply.

3.1.9. Trace an underground circuit

Preconditions:

- The circuit must not be charged;
- Connect the transmitter in a way shown in Fig.3-1-9;
- The earth probe of the transmitter must be properly earthed;
- Select the automatic mode of the receiver;
- Use the displayed signal strength to search or track the circuit.

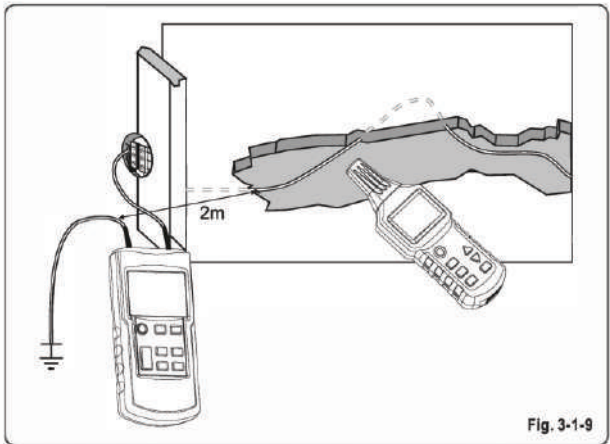


Fig. 3-1-9

1. The distance between the earth probe and the circuit to be searched must be as long as possible. If this distance is too short, the signals and the circuit cannot be located precisely.
2. The depth of detection is greatly influenced by the conditions of the earth. Select suitable receiving sensitivities to precisely locate the circuit.
3. When slowly moving the receiver along the circuit to be searched, you will find the display changing a lot. The strongest signals represent the precise location of the circuit.
4. The longer the distance between the feeding signals (transmitter) and the receiver, the lower the strength of signals, and the shallower the detection.



3.2. Dual-pole Applications

3.2.1 Applications in closed circuits

It can be applied to charged circuits and uncharged circuits:
In uncharged circuits, the transmitter only sends encoding signals to the circuit to be detected.

In charged circuits, the transmitter not only sends encoding signals to the circuit to be detected, but also measures and displays the voltage of the charged circuit.

As shown in Fig.3-2-1.



When connecting charged circuits to the transmitter, please do abide by the safety instructions.

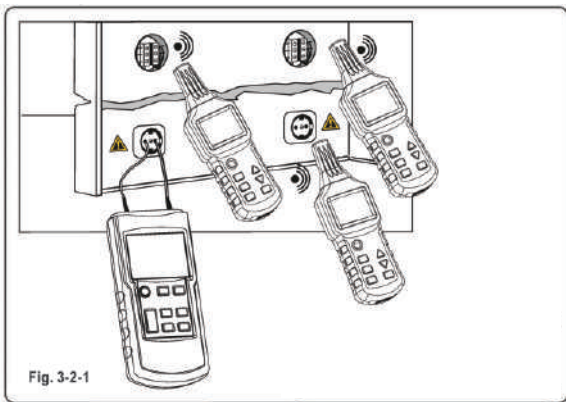


Fig. 3-2-1




1. The dielectric strength of the transmitter is 400v AC/DC.
2. The closed circuit application is suitable for searching sockets, switches and fuses, etc, in the electrical installations of charged or uncharged floors.
3. The depth of detection is related to the media of the cable laid and the way of usage, and the common depth of detection is shorter than 0.5m.
4. Adjust the transmitting power of the transmitter to adapt to different radiuses of detection.

3.2.2 Search for the Circuit Breakers

In a building with multiple residences, use the Land N ports on the socket of any residence to feed the signals from the transmitter (as shown in Fig.3-2-2), and adjust the transmitting power of the transmitter to a suitable level.

Preconditions:

- Turn off all the switches in the distribution box;
- Connect the transmitter according to Fig.3-2-2.

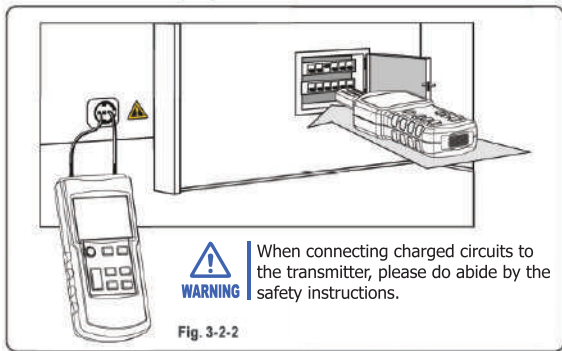

1. The identification and positioning off uses are greatly influenced by the wiring situation in the distribution panel. In order to search for CB or fuses as precisely as possible, one should open or the cover of the distribution panel, and search for the feeder off use.
2. In the searching process, the fuse with the strongest and the most stable signals is the target to be searched for. Due to the coupling of signals, the detector may detect signals from other fuses, but the strengths of those signals are relatively weak.



1. When detecting, it is better to put the probe of detector into the inlet of the DB to achieve the best result of detection.
2. Adjust the transmitting power of the transmitter to adapt to different radiuses of detection. Select the manual mode on the receiver and select suitable receiving sensitivity to precisely locate the circuit.

3.2.3 Search for short circuit in the circuit

Preconditions:

- The circuit must be discharged and disconnected;
- Connect the transmitter according to Fig.3-2-3;
- The measuring method is the same as that shown in the example.

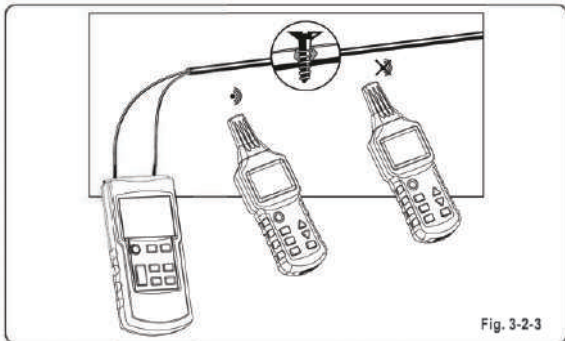


Fig. 3-2-3



1. If there is current in the cable, disconnect the power first and make sure it's discharged.
2. When searching for short circuits of coated electric wires and cables, the depths of detection vary as the core wires are twisted together in the jacket. According to experience, only the short circuits with the impedance lower than 20 ohm can be correctly detected. The impedance of short circuit can be measured with a multimeter.




1. If the impedance of short circuit is higher than 20 ohm, try to use the method to search for breakage in circuit to search for the short circuit. In order to do that, use a relatively high current to temporarily connect the part with the flaw (low ohm connection) or break it.
2. In the process of detecting a long the conduit, if the signals received by the receiver is suddenly attenuated, the detected position is where the short circuit locates.
3. Adjust the transmitting power of the transmitter to adapt to different radiuses of detection.
4. Select the manual mode on the receiver and select suitable receiving sensitivity to precisely locate the circuit.

3.2.4 Detect circuits laid relatively deep

In dual-pole applications, if the loop line is made of core wires in cables with multiple core wires (such as NYM 3x1 .5mm²), the depth of detection will be greatly limited. The reason is that the short distance between the feeding line and the loop line causes a seriously distorted magnetic field. Magnetic field with sufficient strength cannot be built up at the narrow parts. If a separate loop line is used, this problem would be easily solved, as the separate conductor can make the magnetic field diffused more strongly. The loop line may be any kind of conducting wires or cable reels. The important point is that the distance between the feeding line and the loop line must be longer than the depth of laying, and in practice this distance is commonly 2m or longer.

Preconditions:

- The circuit must be discharged and disconnected;
- Connect the transmitter in a way shown in Fig.3-2-4;
- The distance between the feeding line and the loop line must be at least 2-2.5m;
- The measuring method is as shown in the example.

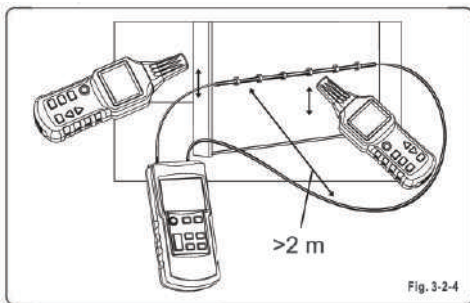

1. In this application, the influence of humidity or mortar on the wall to the depth of locating is insignificant.
2. In the process of detecting the circuit, the stronger the signal displayed on the Receiver of the detector, the closer the cable detected by the detector.
3. Adjust the transmitting power of the transmitter to adapt to different radiuses of detection.
4. Select the manual mode on the receiver and select suitable receiving sensitivity to precisely locate the circuit.



3.2.5. Classify or determine the laid circuit

Preconditions:

- The circuit must be uncharged;
- The ends of core wires must be twisted together and conduct with each other;
- Connect the transmitter in a way shown in Fig.3-2-5;
- The measuring method is the same as that in the example.

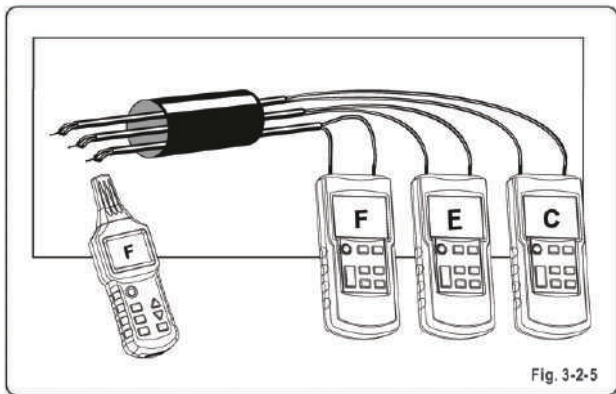


Fig. 3-2-5



CAUTIONS

1. If there is current in the cable, disconnect the power and make sure it's discharged.
2. The ends of core wires without shield must conduct with each other, and must be twisted together.
3. If there is only one transmitter for use, conduct multiple measurements by changing the connection between the transmitter and the cable core wire.



HINTS

1. When changing the connection between the transmitter and cable core wire, different circuits can be distinguished if we change the transmission encoding of the transmitter.
2. Adjust the transmitting power of the transmitter to adapt to different radiuses of detection.
3. Purchase a transmitter with different transmission signals when necessary.

3.3. Method to increase the effective radius of detecting charged circuits

When the transmitter is directly connected to the phase line and neutral line, the signals are conducted on two parallel circuits (as shown in Fig.3-3-1), so the twisting of circuits may sometimes cause signals to counteract each other, leading to an effective radius of 0.5m at most. In order to eliminate this effect, the connection must be as shown in Fig.3-3-2, where the loop line uses a separate cable to increase the effective radius to over 2.5m, and loop lines with longer distances can be provided by the cable reel (see Fig.3-3-2).



When connecting charged circuits to the transmitter, please do abide by the safety instructions.



Pay attention to the distance between the transmitter and the circuit to be detected, in order to clearly determine the circuit through signals.

1. In the process of detecting the circuit, the stronger the signal displayed on the digital tube of the detector, the closer the cable detected by the detector.
2. Adjust the transmitting power of the transmitter to adapt to different radiuses of detection.
3. Select the manual mode on the receiver and select suitable receiving sensitivity to precisely locate the circuit.

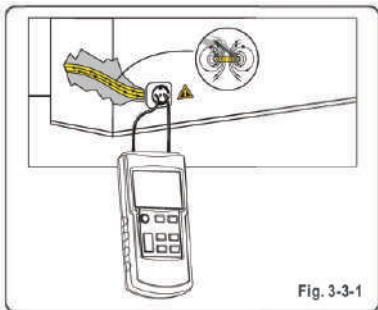


Fig. 3-3-1


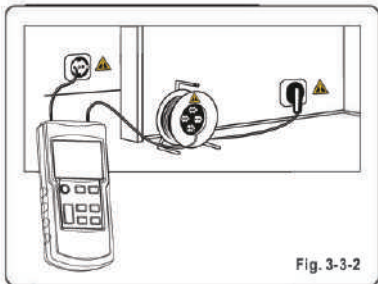


Fig. 3-3-2

3.4. Identify voltage in the grid and search for breakages in the circuit

Preconditions:

- The circuit must be charged with AC voltage;
- The measurement must be conducted according to Fig.3-4;
- Set the transmitter to "Grid Voltage Identification" mode (namely the UAC mode).

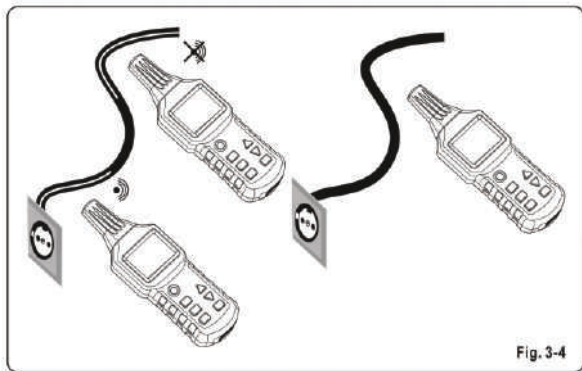

1. The AC signals detected by the transmitter in UAC mode only show that whether the circuit is charged, and the precise measurement of voltage should be done through the voltmeter function of the transmitter.
2. When searching for the ends of multiple power lines, it is necessary to connect each line to the phase line separately.



1. This application does not need the transmitter. (Unless you want to use the voltmeter function of the transmitter to precisely measure the voltage in the circuit.)
2. The signal strength columns displayed on the transmitter and the signal tone frequency are related to the voltage in the circuit to be detected and the distance to the circuit. The higher the voltage and the shorter the distance to the circuit, the more the columns displayed and the higher the signal tone frequency.

4. Other Functions

4.1. Voltmeter function of the transmitter

If the transmitter is connected to a charged circuit and the external voltage is higher than 12V, the lower left part of the monitor of transmitter shows current value of voltage, and standard symbols are used to distinguish AC and DC circuits (see ④, ⑤, ⑥ in the interface displayed on the transmitter), and the upper part of the monitor shows a lightning symbol with a triangular frame (see ⑩) in the interface displayed on the transmitter). The range of identification is 12~400V DC/AC (AC: 50~60Hz).

4.2 Flashlight function

Press the flashlight button ⑨ on the transmitter or flashlight button ⑥ on the receiver to turn on the flashlight function, and press it again to turn off the flashlight function.

4.3 Backlight function

Press the backlight button ⑤ on the receiver to turn on the backlight, and press it again to turn off the backlight. The transmitter does not have the backlight function.

4.4 Mute function

Press the mute button ⑧ on the transmitter to turn off the buzzer, then the buzzer would not make a sound when any button is pressed; press the mute button again to turn off the mute function of the transmitter, and the buzzer function is recovered. Hold on to the backlight/mute button ⑤ on the transmitter for 1 second to turn off the sound, and the buzzer or the speaker of the receiver would not make a sound; Hold on to the backlight/mute button ⑤ on the receiver for 1 second to turn off the mute function, and the functions of buzzer and the speaker of the receiver are recovered.

4.5 Auto power off function

The transmitter has no auto power off function. If any button of the receiver has not been pressed in a relatively long time, the receiver would be automatically turned off in about 10 minutes. Please press the on/off button ② to power on the transmitter.

5. Technical Parameters

5.1. Technical parameters of transmitter

Function	Range
Output signal	125 kHz
External voltage identification range	DC 12~400 V $\pm 2.5\%$; AC 12~400V (50~60Hz) $\pm 2.5\%$
Display	LCD, with function display and column chart
External voltage's dielectric strength	Max. 400V AC/DC
Overvoltage type	CAT III 300V
pollution degree	2
Power supply	1 x 9V, IEC 6LR61
Power consumption - MIN current	About 31mA
Power consumption - MAX current	About 115mA
Fuse	F0.5A 1000V, 6.3X32mm
Range of temperature In work	0°C to 40°C, with maximum humidity of 80% (non condensation)
Range of temperature In storage	-20°C to 60°C, with maximum humidity of 80% (non condensation)
Altitude	Max. 2000m
Dimensions (HxWxD)	190mm x 89mm x 42.5mm
Wieght without battery	About 360g
Weight with battery	About 420g

5.1. Technical parameters of receiver

Function	Range	
Depth of tracking	The depth of tracking depends on the material and specific applications	
Cable locating mode	Single pole application	About 0~2m
	Dual-pole application	About 0~0.5m
	Single loop line	Up to 2.5m
Display	LCD, with function display and column chart	
Power supply	6 x 1.5V AAA, IEC Lr03	
Power consumption - MIN current	About 32mA	
Power consumption - MAX current	About 89mA	
Range of temperature In work	0°C to 40°C, with maximum humidity of 80% (non condensation)	
Range of temperature In storage	-20°C to 60°C, with maximum humidity of 80% (non condensation)	
Altitude	Max. 2000m	
Dimensions (HxWxD)	241.5mm x 78mm x 38.5mm	
Wieght without battery	About 280g	
Weight with battery	About 350g	

6. Repair and Maintenance

1. If the detector is suspected of malfunctioning, please confirm that the electrical amperage of the battery is sufficient and the test lead is not broken.
2. Before sending back the detector for repair, please check the battery. Properly pack the apparatus to avoid damaging it during transportation. For damages caused during transportation, the company would assume no responsibility.
3. There is a fuse within the transmitter. If it is damaged during the guarantee period, it can only be replaced by technical personnel of the company. If it is damaged after the guarantee period, please replace it with a fuse of the same model by yourself. This fuse is single metal wire fast-blow type, so do not replace it with a helical metal wire of delayed type, otherwise the transmitting power and safety of apparatus cannot be guaranteed.

6.1. Troubleshooting

If the detector does not work properly, please check the items in the table below:

Malfunction	Items to be checked	Measures to be taken
Cannot turn on the machine	Has the battery been installed?	Install new batteries
	Is the electrical amperage of the battery too low?	
	Is the polarity of the battery correct?	
Transmitter cannot identify external voltage	Is the contact sound?	Check the polarity
	Transmitter cannot	Reconnect the line
	Is the probe broken?	Replace the probe
	Has the probe been inserted to the bottom?	Properly insert the probe
	Is the test lead broken?	Replace the test lead
Power supply is cut off during measuring	Has the test lead been inserted to the bottom?	Properly insert the test lead
	Is the electrical amperage of battery sufficient?	Replace the battery
The transmitter cannot receive the signals transmitted by itself	Did the machine automatically turn off?	Turn on the machine again
	Has the transmission button been pressed?	Transmit again
	Is the fuse of transmitter broken?	Send it back to a closest service center

6.2. Checking of the fuse of the transmitter

The fuse of the transmitter can prevent the transmitter from being damaged by overload or wrong operations. If the fuse in the transmitter has already been melted down, the transmitter can only transmit weak signals. If the self-check of transmitter is passed but the signal transmitted is weak, it means that the transmission is sound but the fuse has been melted down. If no signal is found during the transmission status self-check of the transmitter, and the voltage of battery is normal, it means that the transmitter is broken and should be repaired by special technicians.

Specific methods and steps to check the fuse of the transmitter:

1. Break all the measuring circuits of the transmitter;
2. Turn on the transmitter and put it in the transmitting status;
3. Set the transmitting power of transmitter to level I
4. Connect one end of the test lead to the joint ⑩ of the transmitter;
5. Insert the other end of test lead into the connecting socket of the transmitter;
6. Turn on the transmitter to search for the signals from the test lead, and move the probe of the receiver towards the test lead;
7. If the fuse is not broken, the value displayed on the receiver will be doubled.

6.3. Cleaning

Use a rag dipped with clean water or neutral detergent to wipe the transmitter, and then use a dry rag to wipe it again.



CAUTIONS

1. Before cleaning work, please make sure that the equipment has been turned off, and all the circuits have been cut off.
2. During cleaning work, please do not use benzene, alcohol, acetone, ether, ketone, thinner or gasoline, which would make the equipment deformed or decolored.
3. After cleaning, use the equipment again when it is completely dry.

6.4. Replace the battery

If the battery symbol on the display flickers

(① of the transmitter or ①, ②, of the receiver), and the buzzer gives warning, then the battery must be replaced.

Steps to replace the battery (of the transmitter or the receiver) are as follows:

1. Turn off the equipment and cut off all the measuring circuits;
2. Unscrew the back of the equipment, and take out the battery cover of the equipment;
3. Take out the battery used up;
4. Install a new battery according to correct polarity;
5. Put back the battery cover and fasten the screws.



WARNING

1. When inserting or replacing the battery, please do pay attention to the correct polarity of battery. If the polarity of battery is incorrect, the equipment will be damaged. Furthermore, explosion or fire may be caused.
2. Do not connect the two poles of the battery with a conducting wire, and do not throw the battery into fire, otherwise there may be risk of explosion.
3. Please do not try to dismantle the battery! The electrolyte contained shows strong basicity, which has the risk of causing corrosion! If the electrolyte contacts skin or clothes, use fresh water to wash the relevant parts. If the electrolyte enters the eyes, use fresh water to wash the eyes immediately, and see a doctor as soon as possible.



1. Before replacing the battery, the equipment must be turned off, all the connected measuring circuits must be cut off, and all the conducting wires for measurement must be removed.
2. Only the battery specified in the technical parameters table can be used.
3. If the equipment will not be used in a relatively long time, take out the battery within it. If the detector is contaminated due to leakage of battery, mail the equipment back to the original factory for cleaning and checking.
4. When disposing the used batteries, please abide by the existing regulations on the recovery, reuse and disposal of batteries.

6.5. Interval of Calibration

In order to ensure the precision of measurement made by the equipment, the equipment should be calibrated regularly by the adjusting personnel of the company. The interval of calibration recommended is one year. If the equipment is used frequently or the conditions of usage are very poor, the interval of calibration should be shortened. If the equipment is rarely used, the interval of calibration can be extended to three years.



MAJOR TECH (PTY) LTD

South Africa

 www.major-tech.com

 sales@major-tech.com

Australia

 www.majortech.com.au

 info@majortech.com.au

